


DIAL INDICATOR TESTER/EXTENSOMETER TESTER




7201-25

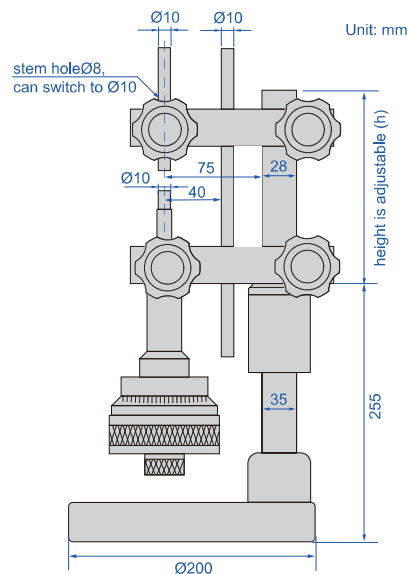

- To calibrate indicators and test indicators with 0.01mm/0.001mm graduation
- To calibrate extensometer with level 0.5 or below
- The height of column is adjustable(h): 150-260mm
- Supplied with dust cover

Code	Micrometer		Accuracy		
	Graduation	Measuring range	Spindle feed error (any 2mm stroke)	Spindle feed error (25mm stroke)	Hysteresis
7201-25	0.2µm	0-25mm	±1µm	±1.5µm	0.5µm

inspect accuracy of extensometers

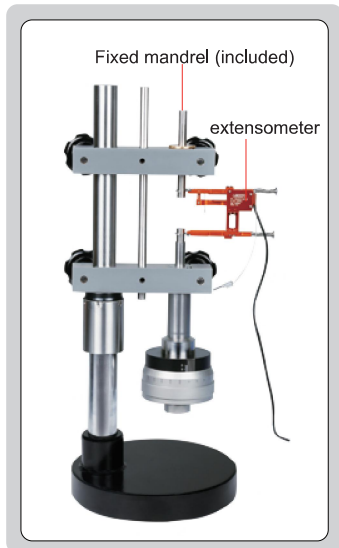

inspect accuracy of digital indicators

